



85um 2016 4-laser (5-2-2-4)

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	
Serial Number:	P18100014	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	12/11/2016 11:50:05 AM
Sheath Pressure:	45.00		
Nozzle Size:	85		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

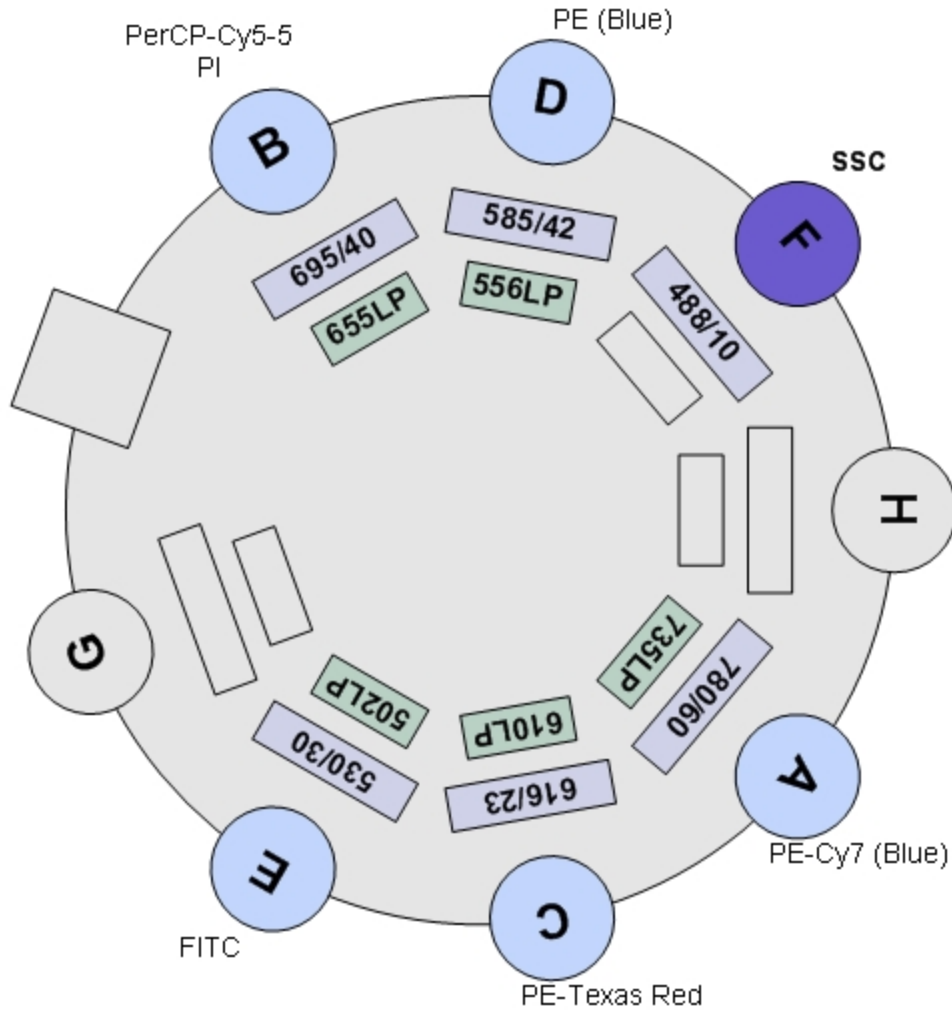


Red Laser
(633nm)

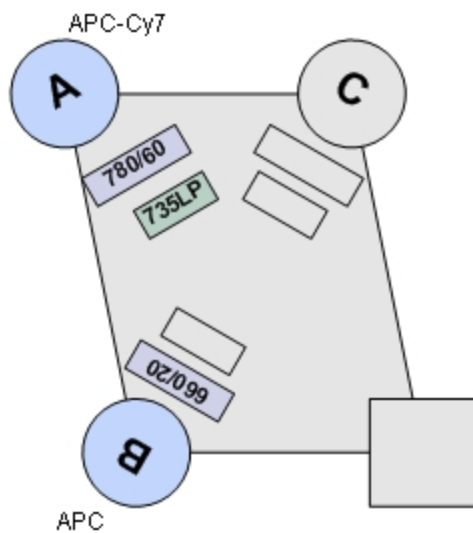

Violet Laser
(407nm)

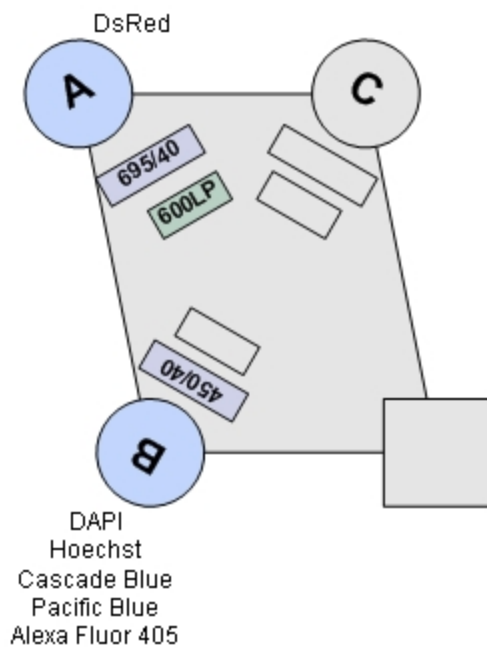

Yellow Green Laser
(561nm)

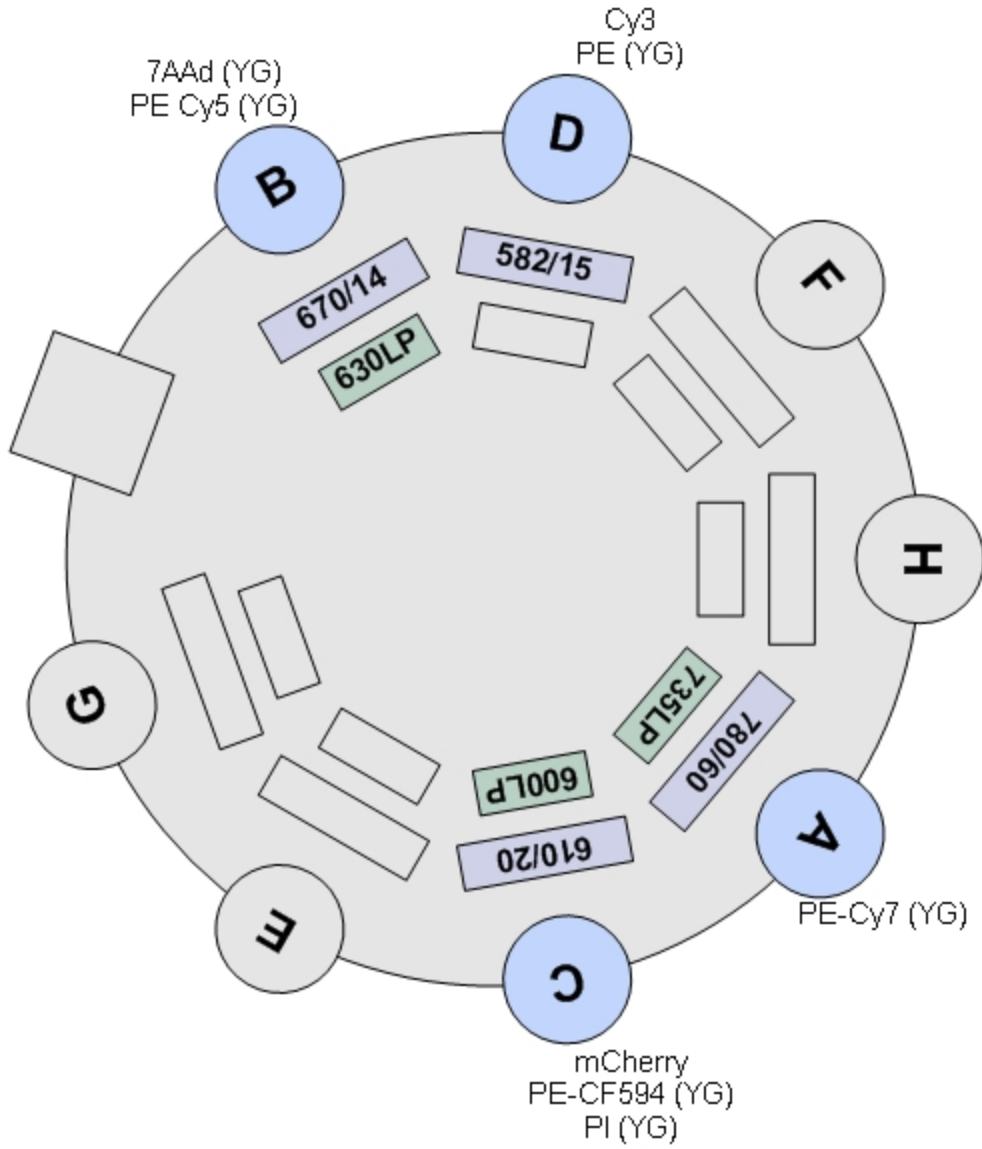

Comments: